



Certificate of Analysis

LudgerSep R2 HPLC Column for Glycan Analysis

Cat. #: LS-R2-4.6x150

Batch #: B6BT-11

Size: 4.6 x 150 mm

This column conforms to the specifications given in Ludger document # LS-R2-GUIDE.

Packed Solvent 60 % acetonitrile (aq)

Test Analysis

Flow Rate 1.25 ml / min


Eluent Isocratic 60 % acetonitrile (aq)

Pressure 1750 psi

Temperature Ambient

Sample Volume 2.5 μ l

Detection UV at 254nm

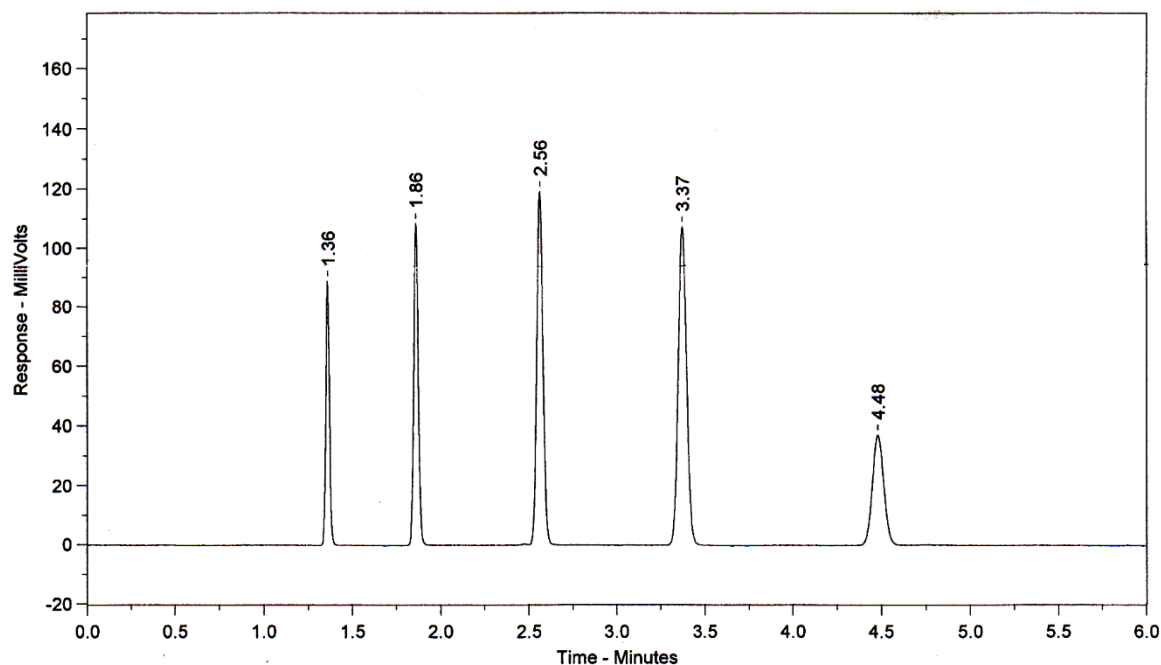

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophylline	1.36	1.10
2	p-Nitroaniline	1.86	1.08
3	Methyl Benzoate	2.56	1.03
4	Phenetole	3.37	1.06
5	o-Xylene	4.48	1.05

Efficiency o-Xylene (n/m) = 153096

Asymmetry Factor (5%) o-Xylene = 1.05