



Certificate of Analysis

LudgerSep UR2 HPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x100

Batch #: B4AA-02

Size: 2.1 x 100 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

Packed Solvent 50 % acetonitrile (aq)

Test Analysis

Flow Rate 500ul / min


Eluent Isocratic 50 % acetonitrile (aq)

Pressure 7343 psi

Temperature Ambient

Sample Volume 1 μ l

Detection UV at 254nm

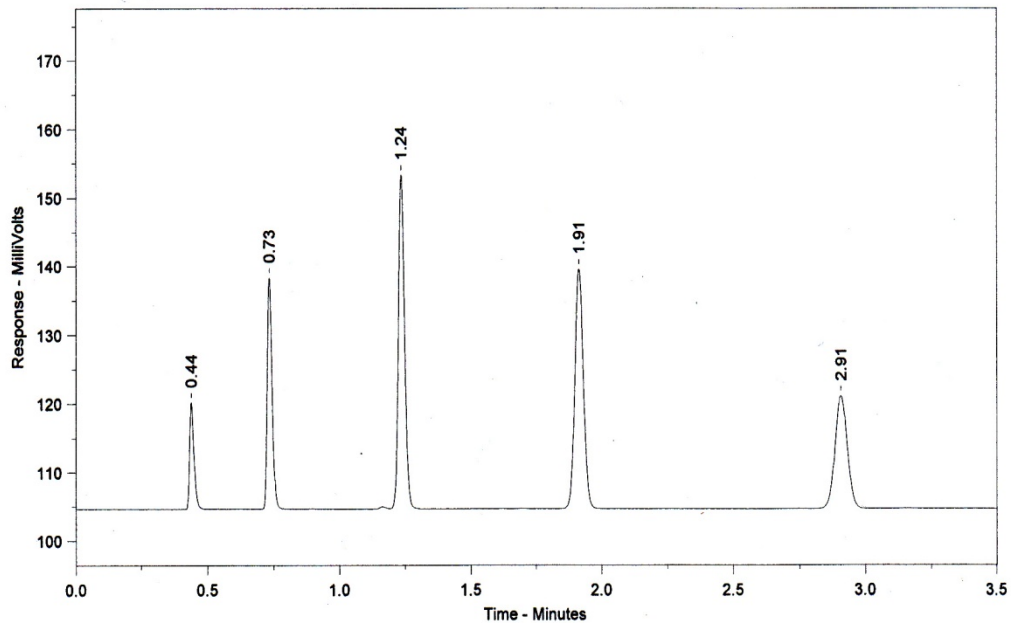

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophyline	0.44	1.44
2	p-Nitroaniline	0.73	1.30
3	Methyl Benzoate	1.24	1.15
4	Phenetole	1.91	1.07
5	o-Xylene	2.91	1.02

Efficiency o-Xylene (n/m) = 175524

Tailing Factor (5%) o-Xylene = 1.02