

## Certificate of Analysis

### LudgerSep™ UR2 UHPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x100

Batch: B8A3-02

Size: 2.1 x 100 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

**Packed Solvent** 50 % acetonitrile (aq)

#### Test Analysis


**Flow Rate** 500ul / min

**Eluent** Isocratic 50 % acetonitrile (aq)

**Pressure** 7086 psi

**Sample Volume** 1 µl

**Detection** UV at 254nm

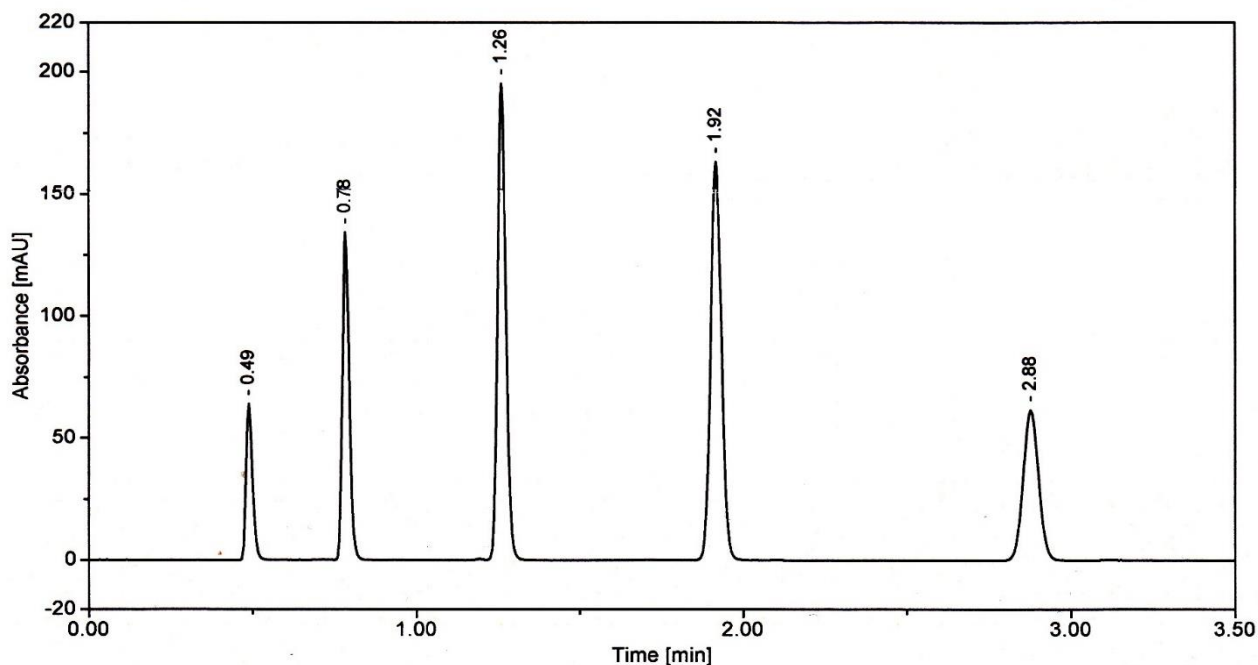

<b>Peak No</b>	<b>Peak Name</b>	<b>Retention time (minutes)</b>	<b>Tailing Factor (5%)</b>
1	Theophylline	0.49	1.35
2	p-Nitroaniline	0.78	1.23
3	Methyl Benzoate	1.26	1.14
4	Phenetole	1.92	1.07
5	o-Xylene	2.88	1.05

**Efficiency o-Xylene (n/m) = 178730**

**Tailing Factor (5%) o-Xylene = 1.05**