



Ludger

Certificate of Analysis

LudgerTag Procainamide Glycan Labelling Kit

Cat. #: LT-KPROC-24

Batch #: B7CD-01

Size: 2 sets of labeling reagents per kit

Expiry date: 14 March 2020

This kit conforms to the specifications given in Ludger document # LT-KPROC-24-Guide.

Each kit contains the following components:

Quantity per Kit	Cat #	Batch #	Component Name
2	LT-ACETIC-DMSO-01	B73E-01	Acetic Acid with DMSO
2	LT-PROC-01	B7C7-02	Procainamide
2	LT-CYANOB-05	B73H-01	Sodium Cyanoborohydride

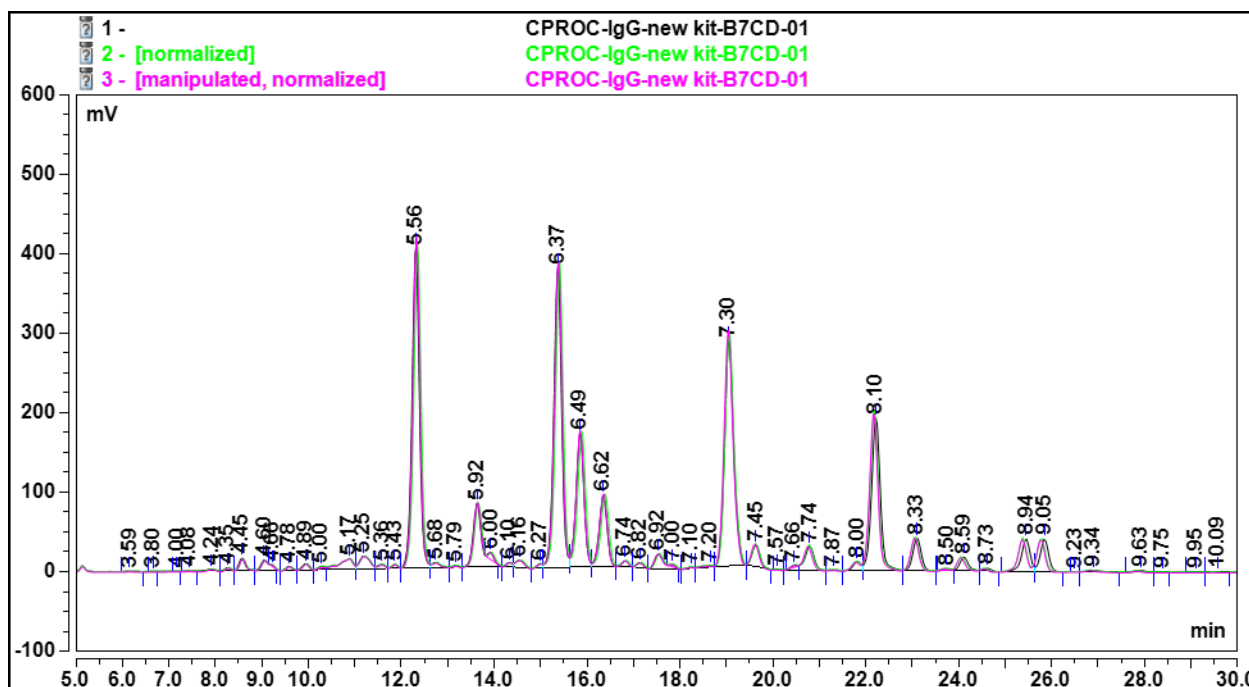


Figure 1: BEH Glycan column UHPLC profile of procainamide labeled N-glycans released from human IgG by PNGase F digestion